

HORIZONTAL – 13.0

September 2006

Third draft

Soils, sludges and treated bio-waste – Organic constituents - LAS by HPLC with fluorescence detection (LC-FLD) and mass selective detection (LC-MSD)

ICS:

Descriptors:

Document type: International Standard
Document subtype:
Document stage: (50) Approval
Document language: E

Contents

Page

Introductionv

1 Scope.....1

2 Normative references.....1

3 Terms and definitions2

4 Principle.....2

5 Interferences3

6 Hazards.....3

7 Reagents.....3

8 Apparatus6

9 Sampling and sample pretreatment6

10 Procedure7

11 Calculation and expression of results.....11

12 Test report12

Annex A (informative) Example of chromatographic conditions and chromatogram 14

Annex B (informative) Clean-up procedure 16

Annex C (informative) Validation 17

Annex D (informative) Information on project Horizontal and WPxx 18

Bibliography..... 19

Foreword

This document has been prepared in the framework of the project Horizontal.

This document is a working document.

The following TC's have been involved in the preparation of the standard: CEN/TC 292, CEN/TC 308 and ISO/TC 190.

This standard is applicable and validated for several types of matrices. The table below indicates which ones.

Material	Validated	Document
Soil	<input type="checkbox"/>	[reference]
Sludge	<input type="checkbox"/>	
Treated bio-waste	<input type="checkbox"/>	
Soil improvers	Not validated yet	
Waste		

Introduction

This document is developed in the framework of the project 'Horizontal'. It is the result of a desk study “LAS and Nonylphenols” from January 2004 /1/ and an extensive experimental study of the method including a ruggedness test /2/. During the development of the horizontal method, the work has been discussed by an ad-hoc group formed to facilitate such discussions. The ad-hoc group have had five meetings during the period September 2003-September 2005, all meetings held in conjunction with other standardisation committee meetings in CEN/TC 308/WG 1 and ISO/TC 190.

The anionic surfactant LAS (Linear Alkylbenzene Sulfonates) is found in the environment due to the use of LAS in detergents. For more than 30 years LAS has been the largest single surfactant used in detergents, and the use continues on a high level.

Although LAS is readily biodegradable during wastewater treatment, considerable amounts may still be found in sludges of municipal origin. By the use of sludge for soil enrichment LAS may end up in the agricultural soil, where a rapid biodegradation takes place.

The method describes the determination of LAS in sludge, soil, treated biowaste and neighbouring fields. LAS is the sodium salt of alkylbenzene sulfonic acids, and it consists of a mixture of the homologues C₁₀-LAS, C₁₁-LAS, C₁₂-LAS, C₁₃-LAS and C₁₄-LAS. LAS is determined as the sum of the homologues.

The texts of the chapters are normative; annexes are normative or informative, as stated in the top lines of the annexes.

Soils, sludges and treated bio-waste – Organic constituents - LAS by HPLC with fluorescence detection (LC-FLD) and mass selective detection (LC-MSD)

1 Scope

This European standard describes a method for the determination of Linear Alkylbenzene Sulphonate (LAS) in soil, sludge and treated bio-waste using HPLC with a fluorescence detector or a mass selective detector.

The standard primarily describes the analysis of sludge, soil and treated bio-waste. Other solid materials like sediment and selected solid wastes may also be analysed by the method, provided the required validation has been performed.

The standard describes the determination of the sum of LAS. Under the conditions specified in this standard, typically a limit of detection of 20 mg/kg (expressed as dry matter) for sludge and of 0,2 mg/kg for soil and treated bio-waste may be achieved.

Temporary remark: The exact LOD will be determined by the method validation.

Matrices for which the standard has been validated are listed in the foreword.

Lower LOD's may be achieved by concentrating the extract by solvent evaporation.

NOTE The single LAS homologues C₁₀ – C₁₄ can be determined by the standard.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, only the edition cited applies. For undated references, the latest edition of the normative document referred to applies (including any amendments).

ISO/DIS 10381-1, *Soil quality – Sampling – Part 1: Guidance on the design of sampling programmes.*

ISO/DIS 10381-2, *Soil quality – Sampling – Part 2: Guidance on sampling techniques.*

ISO/DIS 10381-8, *Soil quality – Sampling – Part 8: Guidance on sampling of stockpiles.*

Horizontal standard 2-2, *Sampling of sludges and treated bio-wastes.*

Horizontal standard 2-3, *Sampling of soils.*

ISO 11465:1993, *Soil quality – Determination of dry matter and water content on mass basis – Gravimetric method.*

PrEN 14346, *Characterisation of waste – Calculation of dry matter by determination of dry residue and water content.*

EN 12880, *Characterisation of sludge – Determination of dry residue and water content.*

LAS standard – Horizontal – 13.0

Horizontal standard 17-1 (draft), *Solid materials – Determination of dry matter and water content on a mass basis – Gravimetric method.*

ISO/DIS 14507, *Soil quality – Guidance for sample pre-treatment for the determination of organic contaminants in soil.*

ISO/DIS 16720:2003, *Soil quality – Pre-treatment of samples by freeze-drying for subsequent analysis.*

Horizontal standard 33-2, *Solid materials – Pre-treatment for organic characterisation.*

ISO/FDIS 22982:2004, *Soil quality – Guidelines for the identification of target compounds by gas chromatography and mass spectrometry*

ISO 8466-1, *Water quality – Calibration and evaluation of analytical methods and estimation of performance characteristics.*

3 Terms and definitions

3.1 Analyte

In the context of this international standard, the analyte is linear alkylbenzene sulfonate, sodium salt (LAS). The analyte consists of a mixture of homologues (i.e. C₁₀-LAS, C₁₁-LAS, C₁₂-LAS, C₁₃-LAS and C₁₄-LAS) where each homologue consists of a mixture of 4-6 isomers depending on the length of the alkyl group. The dominant homologues in detergents and environmental samples are C₁₁-LAS and C₁₂-LAS.

NOTE C₁₀-C₁₄ refers to the chain length of the linear alkyl group.

3.2 Calibration standard

A solution prepared from stock solutions of LAS homologues and used to calibrate the response of the instrument with respect to analyte concentration.

3.3 Internal standard

The 4-octylbenzenesulfonate (C₈-LAS) is added to the test sample before extraction. The internal standard is used to correct for losses during the analytical procedure and is used for calculating the concentration of the analytes.

3.4 Test sample

The test sample is the sample after pre-treatment such as homogenisation, grinding, sieving, drying, etc. The test sample is ready for the chemical analysis.

4 Principle

After pre-treatment according to the methods referred to in chapter 9, the test sample (freeze-dried) is extracted by shaking with methanol. If necessary interfering compounds are removed from the extract by a clean-up on a suitable column.

The extract is analyzed by high performance liquid chromatography (HPLC) on a C₈- or C₁₈-column and detection by fluorescence (FLD) or mass spectrometry (MSD).

The identification is based on the retention times of the homologues and of the isomers of each homologue. Another identification point is the pattern/fingerprint of the homologues, and the isomer fingerprint of each homologue, if a C₁₈-column is used for HPLC. By use of MS detection the relative intensities of two diagnostic ions may also be used for the identification (optional).

The quantification is based on internal standard procedure. The internal standard (C₈-LAS) is taken through the whole analytical procedure.

5 Interferences

5.1 Interferences from sampling

Use sampling containers of materials (preferably glass or steel) that do not significantly affect the sample during the contact through sampling and storage. Plastic containers may be used, if they have been proven not to significantly affect the sample.

5.2 Interferences by LC-FLD and LC-MSD

The chromatographic analysis can be done on a C₈ or a C₁₈ reverse phase column, and the choice of column will determine the separation obtained. On the C₈ column (with methanol in mobile phase) the LAS homologues are separated, however, there is no separation of the isomers. On the C₁₈ column (with acetonitrile in mobile phase) the homologues are separated and there is a partial separation of the isomers of each homologue. This is illustrated by the chromatograms in Annex A.

The selectivity of the fluorescence as well as the mass selective detector is high, however, interference from co-eluting substances may occur. It is essential that the interfering peaks are not included in the calculations. A peak is excluded, if the retention time differs from the LAS standard mixture. Interfering peaks may best be detected when a C₁₈ column is used, due to the partial separation of the isomers. The C₁₈ column is mandatory when fluorescence is used, due to the higher selectivity obtained. The interfering peaks can normally be detected by comparing the fingerprints of the sample with the fingerprints of the LAS standard mixture, although the isomer- and homologue-distribution in the environmental samples may differ from the distribution in the standard mixture.

The highest selectivity is obtained by the use of a C₁₈ column and the MS detector. However, for most applications the separation on a C₈ column is sufficient, when MS is used. When all isomers are eluted in one peak, the integrations are less complicated, resulting in a higher precision and a lower limit of detection.

Depending on the type of matrices from which LAS is extracted different analytical pathways can be applied. An overview of the analytical procedure for the matrix of interest is shown in the table below.

Table 1: Choice of analytical procedure.

	FLD		MSD	
	C8-column	C18-column	C8-column	C18-column
Sludge	No	Yes	Yes	Yes
Soil	No	(Yes) [#]	Yes	Yes
Treated Bio-waste	No	(Yes) [#]	Yes	Yes

#) For FLD the LOD will generally be inadequate for this type of matrix.

6 Hazards

7 Reagents

All reagents shall be of recognised analytical grade.

LAS standard – Horizontal – 13.0

The purity of the reagents used shall be checked by running a blank determination as described in 10.4. If the blank value is unreasonably high, i.e. more than 10 % of the lowest value of interest, find the cause through a step-by-step examination of the whole procedure.

7.1 Methanol, CH₃OH

HPLC-grade.

7.2 Acetonitrile, C₂H₃N

HPLC-grade.

7.3 Ammonium acetate, [CH₃COO⁻ NH₄⁺]

7.4 Mobile phases for HPLC

For isomeric separation on C₁₈ column:

Mobile phase A: 0.01 M ammonium acetate

Mobile phase B: acetonitrile

For homolog separation on C₈ column:

Mobile phase A: 0.01 M ammonium acetate

Mobile phase B: methanol

7.5 Reagents for clean-up procedures

7.5.1 Clean-up procedure based on Strong anion exchange (SAX)

7.5.1.1 SAX column

7.5.1.2 Acetic acid (CH₃COOH)

7.5.1.3 Hydrochloric acid (HCl)

7.5.1.4 Methanol

7.5.2 Clean-up procedure based on Graphitised carbon black (GCB)

7.5.2.1 GCB column

7.5.2.2 Hydrochloric acid (HCl)

7.5.2.3 Tetramethylammonium hydroxide (CAS# 10424-65-4)

7.5.2.4 Formic acid (HCOOH)

7.5.2.5 Dichloromethane

7.5.2.6 Methanol

7.6 Nitrogen for solvent evaporation

Nitrogen of sufficient purity.

7.7 Standards for calibration

7.7.1 C₁₁ LAS, Sodium Linear Undecylbenzene Sulfonate C₁₇H₂₇SO₃Na, 99%

7.7.2 C₁₂ LAS, Sodium Linear Dodecylbenzene Sulfonate C₁₈H₂₉SO₃Na, 99% (CAS# 2211-98-5)

7.7.3 C₁₃ LAS, Sodium Linear Tridecylbenzene Sulfonate C₁₉H₃₁SO₃Na, 99%

7.7.4 C₁₀-C₁₄ LAS mixture of homologues and isomers, highest possible purity, (CAS # 69669-44-9, CAS # 25155-30-0)

7.8 Internal standard, C₈-LAS

Octylbenzene sulfonic acid, sodium salt C₁₄H₂₁SO₃Na, CAS # 6149-03-7

The internal standard must be kept in the freezer.

7.9 Internal standard solution

Prepare internal standard solution by dilution to about 1000 mg/l in methanol.

It is essential, that the same internal standard solution is used for calibration standard solutions and for samples, blank and internal quality control samples.

NOTE Store the internal standard solution in a dark place at a temperature of less than 4 ± 3 °C. The solution is stable for at least 2 years.

7.10 Stock solutions

Prepare individual stock solutions of 1000 - 5000 mg/l in methanol, either from solid standard substances or from solutions with a certified concentration. Prepare stock solutions of C₁₁ LAS (7.7.1), C₁₂ LAS (7.7.2) and C₁₃ LAS (7.7.3).

Prepare a calibration mixture by mixing stock solutions of C₁₁ LAS, C₁₂ LAS and C₁₃ LAS obtaining equal concentration of each homologue.

Prepare a stock solution of C₁₀ – C₁₄ LAS mixture (7.7.4) of 1000 – 5000 mg/l in methanol. This solution is only for identification.

NOTE Store the stock solutions and the calibration mixture in a dark place at a temperature of 4 ± 3 °C. The solutions are stable for at least 2 years.

7.11 Calibration standard solutions

Calibration standard solutions are prepared from the calibration mixture by diluting with methanol. The calibration range is different for sludge and for soil/sediment/treated bio-waste.

7.11.1 Sludge

For sludge samples the calibration standards are made to concentrations from 5 mg/l to 500 mg/l. The internal standard solution is added to a concentration of 10 mg/l.

7.11.2 Soil, sediment and treated bio-waste

For samples of soil, sediment or treated bio-waste the calibration standards are made to concentrations from 0,05 mg/l to 5 mg/l. The internal standard solution is added to a concentration of 1 mg/l.

NOTE 1 Store the calibration standard solutions in a dark place at a temperature of less than 4 ± 3 °C.

LAS standard – Horizontal – 13.0

NOTE 2 A diluted C₁₀ – C₁₄ mixture is prepared for the identification of the C₁₀ and C₁₄ homologues, which are not present in the calibration mixture.

8 Apparatus

All equipment which gets into contact with the sample or extract shall be free from LAS. Glassware may be cleaned by heating, at least for 2 hours at 450°C.

8.1 Standard laboratory glassware

Screw cap glass flask with PTFE seal. Volume 20 ml and 100 ml.

Round-bottomed flasks. Volume 100 ml and 250 ml.

Test tubes and vials.

8.2 Shaking device

Reciprocating shaker with horizontal movement (up to at least 250 strokes per minute).

8.3 Evaporator

Rotary evaporator. Other device like turbo evaporator or Kuderna Danish may be applied.

8.4 Freeze drying apparatus

8.5 (High-performance) liquid chromatograph with fluorescence or mass selective detector

The HPLC system is equipped with a C8 or C18 reverse phase chromatographic column. The dimensions should be sufficient to separate the LAS as described below. Two examples of LC- columns are given in Annex A.

The fluorescence detector shall be able to measure at excitation wavelength of 230 nm and emission wavelength of 310 nm. If a fixed wavelength detector is used, the nearest possible wavelengths shall be used.

The mass selective detector shall be equipped with an API-ES interface (atmospheric pressure ionization electro-spray). The negative ion mode is used.

The separation of LAS homologues must fulfil the following requirements: The five homologues C₁₀ – C₁₄ shall all be separated to baseline.

Isomeric separation (mandatory for fluorescence detection): C₁₁-LAS shall be separated into at least 4 chromatographic peaks, although these are not separated to baseline.

9 Sampling and sample pretreatment

9.1 Sampling and sample storage

Obtain representative samples in accordance with ISO 10381-1 (soil) using sampling apparatus in accordance with ISO 10381-2. Use Horizontal standard 2-2 for sampling of sludge and biowaste.

Store the samples in a dark place at a temperature below 10°C, if possible in a refrigerator. Determine the content of dry matter in the sample in according to EN 12880, ISO 11465 or PrEN 14346 – **Temporary remark: Horizontal standard 17-1.**

NOTE Freeze-dried samples, if kept sealed, may be stored for a longer period at room temperature (approx. 1 month). Hygroscopic dried sludge may be preserved by mixing with anhydrous sodium sulphate.

9.2 Sample pre-treatment

Samples shall be pre-treated as soon as possible after sampling.

Methods for pre-treatment of solid samples to be used for the analysis of organic contaminants are described in a separate standard, Horizontal standard 33-2. This standard describes procedures for the preparation of the test sample from the laboratory sample.

All samples are dried, preferably by freeze-drying. Conventional drying at 60°C can be used, however, conventional drying may result in crusty hard samples that are difficult to homogenize.

10 Procedure

10.1 Extraction

Two extraction methods are described – one for extraction of sludge samples and one for extraction of samples of soil, sediment and treated bio-waste.

All types of solids (sludge, soil, sediments and treated bio-waste) are dried and extracted with methanol.

10.1.1 Extraction of dried sludge

Dried sludge samples are extracted as follows:

- a) Weigh accurately 2-3 g (with 2 decimals) of test sample and place it in a screw cap flask (20-100 ml) with PTFE seal.
- b) Add 100 µl of internal standard solution (7.7) equal to 100 µg of internal standard.
- c) Add 10 ml of methanol, close the screw cap and place the flask on the horizontal shaker. The flask shall be placed in horizontal position.
- d) Shake for at least 30 minutes with 250 ± 20 strokes per minute.
- e) Wait for sample to settle, then transfer 500 µl of extract to a vial and add 500 µl of 0.01M ammonium acetate (mobile phase A) (7.4)
- f) The extract is now ready for analysis by LC

By high LAS concentrations less sample can be taken into analysis.

10.1.2 Extraction of dried soil, sediment and treated bio-waste

Dried soil, sediment and treated bio-waste samples are extracted as follows:

- a) Weigh accurately 10-15 g (with 2 decimals) of test sample and place it in a 100 ml screw cap flask with PTFE seal.
- b) Add 50 µl of internal standard solution (7.7) equal to 50 µg of internal standard.
- c) Add 50 ml of methanol, close the screw cap and place the flask on the horizontal shaker. The flask shall be placed in horizontal position.

LAS standard – Horizontal – 13.0

- d) Shake for at least 60 minutes with 250 ± 20 strokes per minute.
- e) Wait for sample to settle, then transfer 500 μl of extract to a vial and add 500 μl of 0.01M ammonium acetate (mobile phase A) (7.4)
- f) The extract is now ready for analysis by LC.

The extracts can be stored in a refrigerator ($4^{\circ}\text{C} \pm 3^{\circ}\text{C}$).

NOTE Other extraction techniques, like ultrasonic extraction, soxhlet, reflux, microwave or pressurised liquid extraction may be suitable. However if using other extraction techniques the comparability to the method described in this standard shall be proven.

10.2 Concentration (optional)

In most cases concentration of the extract is not necessary. However, if lower detection limits are needed this can be achieved by the evaporation of the solvent.

Concentrate the extract on a rotary evaporator or by the use of a gentle stream of nitrogen at room temperature. Since the internal standard is used for the calculations, it is not necessary to know the exact volumes. If necessary the amount of internal standard added to the sample can be reduced relative to the concentration factor to keep the concentration of internal standard at the same level in the analysis.

10.3 Clean-up (optional)

Clean-up has to be used if compounds are present that can interfere with the analytes or the internal standard in the chromatography, or if those compounds can influence the HPLC-procedure (i.e. contamination of the detection system). If no or negligible interfering substances are present, no clean-up is necessary.

The selectivity of the mass selective detector (MSD) is higher than of the fluorescence detector (FLD), and the clean-up is therefore mostly used for the FLD. For the MSD a clean-up is generally not necessary.

For sludge samples a clean-up is generally not necessary, disregarding the choice of detector.

Add a proportion of the extract to the clean-up column (7.5.1.1 or 7.5.2.1) and elute the column with a suitable solvent.

Before use the column shall be tested with a calibration standard to ensure that the LAS homologues are recovered in the collected fraction. The criteria for the clean-up is, that the recovery for LAS is higher than 80%.

Two columns are described for clean-up. Descriptions of the clean-up procedures are given in Annex B.

10.4 Blank

Perform a blank determination following the procedure as described for the selected extraction and clean-up (optional). Prepare the blank exactly as by the analysis of a sample. .

The blank value shall not be higher than 10 % of the lowest value of interest.

10.5 HPLC-analysis

Two types of columns (C_8 and C_{18}) and many HPLC-conditions may be used. The choice of column and detector will depend on the matrix to be analysed. This is further described in Table 1 in 5.2. By the use of FLD only C_{18} columns are allowed, by MSD both columns are allowed. Examples are described in Annex A.

Optimise the HPLC-system including the detector according to the instrument manufacturer's manual. The separation of LAS-homologues/isomers must fulfil the requirements described in 8.5.

10.5.1 Fluorescence detection

Optimise the fluorescence detector according to the instrument manufacturer's manual.

If a scanning fluorimeter is used, an initial scan of both excitation and emission wavelength are advisable if detector is not calibrated.

The following wavelengths are used:

Excitation: 230 nm

Emission: 310 nm

10.5.2 Mass selective detection

An API-ES interface set in the negative ion mode is used.

The following ions are used for the analysis:

Table 2 — Diagnostic ions used by the LC-MS analysis

Compound	Abbreviation	Target ion
		M₁
Analytes:		
C ₁₀ -Linear alkylsulfonate	C ₁₀ -LAS	297
C ₁₁ -Linear alkylsulfonate	C ₁₁ -LAS	311
C ₁₂ -Linear alkylsulfonate	C ₁₂ -LAS	325
C ₁₃ -Linear alkylsulfonate	C ₁₃ -LAS	339
C ₁₄ -Linear alkylsulfonate	C ₁₄ -LAS	353
Internal standard:		
C ₈ -Linear alkylsulfonate	C ₈ -LAS	269

NOTE 1 As an option the fragment ion 183 may be used as qualifier ion for the identification (for all homologues). However, for routine use the fragment ion 183 has a low abundance relative to the target ion, and a much higher fragmentor voltage is therefore required.

NOTE 2 C₈-C₁₄ indicate the length of the alkyl chain.

10.6 Calibration and analysis of samples

Two types of calibration are used: the initial calibration (10.6.1) and the recalibration, which is carried out daily (10.6.2).

The initial calibration serves to establish the linear working range of the calibration curve. This calibration is performed when the method is used for the first time and after maintenance and/or repair of the equipment.

LAS standard – Horizontal – 13.0

The recalibration checks the validity of the linear working range of the initial calibration curve and is performed before each series of samples.

For all calibrations the relative areas are used, i.e. the area for the analyte relative to the area for the internal standard. This is described in 11.1.

For LAS the area is determined as the sum of the peak areas of mixtures of homologues (from C₁₀ to C₁₄) and mixtures of isomers. This is the case for measurements with both detectors.

10.6.1 Initial calibration

Inject at least 5 standard solutions with concentrations within the working range described in 7.11. For sludge the working range is from 5 mg/l to 500 mg/l. For soil, sediment and treated bio-waste the working range is from 0,05 mg/l to 5 mg/l. The actual working range may however differ depending on the matrix and the values of interest. Include a solvent blank. Identify the peaks and add the integrated areas of the LAS peaks to give the sum area for LAS. Prepare a calibration curve.

Evaluation of the calibration curve shall be done according to the description in ISO 8466-1. This standard for linear calibration gives acceptance and rejection criteria for linearity.

Note It is allowed to use non-linear calibration using all 5 standards. In that case, all 5 standards shall be used for recalibration and not only the 2 standards described below.

10.6.2 Recalibration

Inject at least two calibration standards with concentrations of $20 \pm 10\%$ and $80 \pm 10\%$ of the established linear range and calculate the straight line from these measurements.

10.6.3 Analysis of samples and identification

Inject the extracts of samples and blanks obtained from the extraction in 10.1, from 10.2 (concentration) or from 10.3 (clean-up).

The identification of LAS is using the following identification points:

- The peak pattern of the homologues, i.e. the fingerprint, although the relation between the individual peaks may differ in samples and standards
- The peak pattern of the isomers of each homologue (only if a C₁₈ column is used)
- The retention times of the individual peaks
- The relation between peak areas of the qualifier ions and the target ion (only by MS-detection, optional)

From the identification select the peaks to be included in the sum area. Peaks not found in the calibration standard are not included. See about interferences in chapter 5.

Use ISO/FDIS 22982 for identification of LAS.

The C₁₀ – C₁₄ LAS mixture is only used to determine the retention times of C₁₀ LAS and C₁₄ LAS, which are not present in the calibration standard.

If the concentration of LAS is out of the calibration range (higher than the upper calibration limit), the analysis shall be repeated with a smaller amount of sample.

11 Calculation and expression of results

For linear alkylbenzene sulphonate (LAS) the areas are determined as the sum of the peak areas of the homologue and isomeric mixtures. If interfering peaks are present, these shall not be included in the sum area.

The method is based on internal standard calculations. The method determines the mass concentrations and is not influenced by injection errors, the volume of water present in the sample or matrix effects in the sample, provided that the recovery of the analyte is about equal to that of the internal standard.

For all samples a specific mass of internal standard is added, 100 µg for extraction method 10.1.1 and 50 µg for extraction method 10.1.2. The recovery of the internal standard must be 60-120 % to ensure an acceptable quality of the performed analysis. This may be checked against the internal standard in the calibration standard solutions.

11.1 Calibration

From the chromatograms of the calibration standards obtain a calibration curve by plotting the ratio of the mass concentrations against the ratio of the peak areas using equation (1):

$$\frac{A_c}{A_{is,c}} = s \cdot \frac{\rho_c}{\rho_{is,c}} + b \quad (1)$$

where:

- A_c is the response of analyte in the calibration standard = sum of peak areas
- $A_{is,c}$ is the response of internal standard in the calibration standard = peak area
- s is the slope of the calibration function
- ρ_c is the mass concentration of analyte in the calibration standard solution in µg/ml
- $\rho_{is,c}$ is the mass concentration of internal standard in the calibration standard solution in µg/ml
- b is the intercept of the calibration curve with the ordinate

11.2 Calculation

From the chromatograms of the samples and blanks calculate the mass concentrations of the analytes from the calibration curve using equation (2):

$$\omega_s = \frac{(A_s / A_{is,s}) - b}{s \cdot m \cdot d_s} \cdot \rho_{is,s} \cdot V \quad (2)$$

where:

- ω_s is the concentration of analyte found in the sample in mg/kg dry matter
- A_s is the response of analyte in the sample = sum of peak areas

LAS standard – Horizontal – 13.0

- $A_{is,s}$ is the response of internal standard in the sample = peak area
- b is the intercept of the calibration curve with the ordinate
- s is the slope of the calibration function
- m is the mass of the test sample used for extraction in grams
- d_s is the dry matter content of the test sample in g/g
- $\rho_{is,s}$ is the mass concentration of internal standard in the sample extract in $\mu\text{g/ml}$
- V is the volume of petroleum ether used for extraction of the test sample, in ml

12 Test report

The test report shall contain at least the following data:

- a) the information required to identify the sample;
- b) a reference to this international standard;
- c) the contents of the analytes in mg/kg dry matter, with two significant figures.
- d) any details not specified in this International Standard or which are optional, as well as any factor which may have affected the results.

Annex A (informative)

Example of chromatographic conditions and chromatogram

Isomeric separation of LAS

HPLC-conditions:

Separation column: Type: C18-column. Particle size: 5µm. Dimensions: 150 x 2,0 mm (other column dimensions such as 150 x 4,6 mm have also proven adequate).

Mobile phase : A) 0,01M ammonium acetate in water, B) Acetonitrile


Solvent gradient:

t (min)	% B
0	45
20	55
35	65
36	95
40	95
41	45
46	45

Inj volume: 25 µl

Flow: 0,2 ml/min

Example of chromatogram obtained with fluorescence detection:

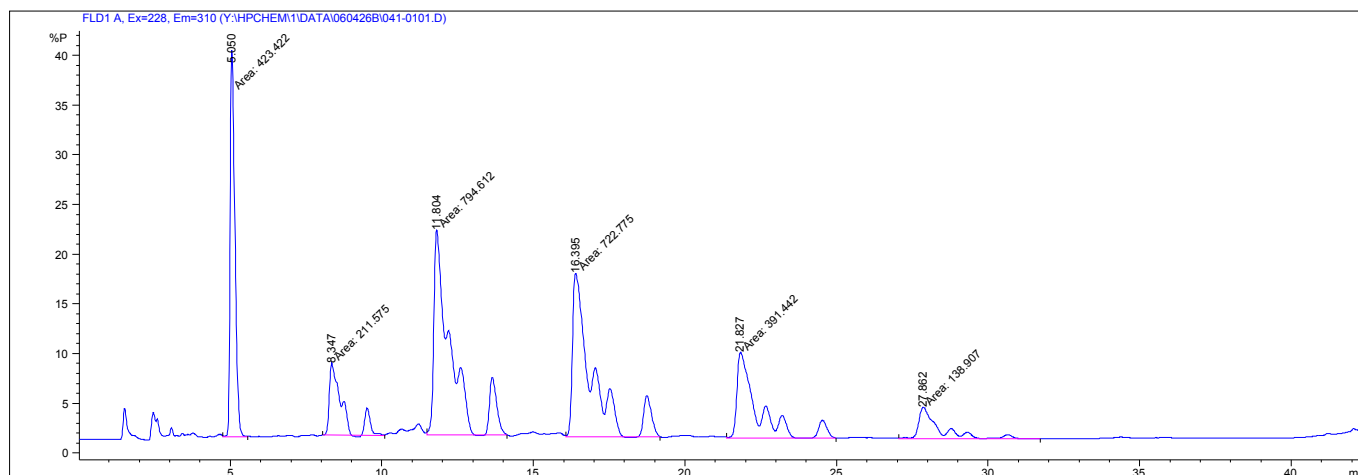

Homologue separation of LAS

HPLC-conditions:

Separation column: Type: C8-column. Particle size: 5µm. Dimensions: 125 x 2,0 mm (other column dimensions such as 125 x 4,6 mm have also proven adequate).

Mobile phase : A) 0,01M ammonium acetate in water, B) MeOH


Solvent gradient:

t (min)	% B
0	58
12	80
16	95
18	95
19	58
25	58

Inj volume: 25 µl

Flow: 0,2 ml/min

Example of chromatogram obtained with fluorescence detection:

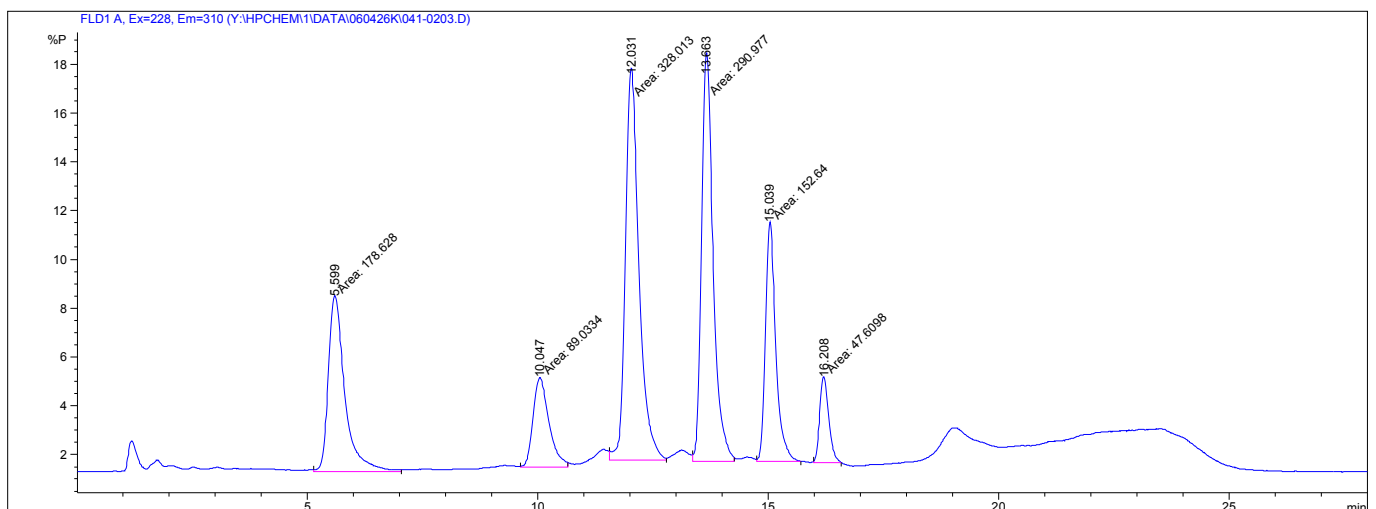

Annex B (informative)

Clean-up procedure

Clean-up procedure based on graphitised carbon black (GCB) columns:

- Type of column: 500 mg pre-packed GCB solid phase extraction (SPE) column.
1. Column preparation: 5 ml mobile phase
2 ml methanol
30 ml 0,1 M hydrochloride acid
2. Sample application: 1 ml MeOH extract
3. Wash: 5 ml water
5 ml methanol
10 ml dichloromethane/methanol (80:20) with 15 mM formic acid
10 ml dichloromethane
4. Elution: 10 ml dichloromethane/methanol (80:20) with 5 mM tetramethylammoniumhydroxide
5. Solvent transfer: Evaporate until dryness and re-dissolve in methanol/mobile phase (1:1).

Clean-up procedure based on strong anion exchange (SAX) columns:

- Type of column: 500 mg pre-packed SAX solid phase extraction (SPE) column.
1. Column preparation: 5 ml methanol
10 ml water
2. Sample application: 1 ml MeOH extract
3. Wash: 5 ml 2% acetic acid in methanol
5 ml methanol
4. Elution: 15 ml 2 M hydrochloride acid:methanol (1:1)
5. Solvent transfer: Neutralize with ammonium acetate, evaporate until dryness and re-dissolve in methanol/mobile phase (1:1).

Annex C (informative)

Validation

Annex D (informative)

Information on project Horizontal and WPxx

Bibliography

1. Gro Fremmersvik and Nis Hansen. Desk Study – LAS and Nonylphenols. January 2004.
<http://www.ecn.nl/horizontal/>.
2. Rune Haller and Nis Hansen. LAS – Experimental work including ruggedness test. August 2006.
<http://www.ecn.nl/horizontal/>.